

# Human FKBP1B ELISA Kit

**Cat: RK00085**

This ELISA kit used for quantitation of human Peptidyl-Prolylcis-Transisomerase Fkbp1B (FKBP1B) concentration in cell culture supernate, serum and plasma. For research use only, and it's highly recommended to read throughly of this manual before using the product.

## Manufactured by

**Global Headquarters**

**86 Cummings Park**

**Woburn, MA 01801**

**Tel: +8887545670**

**China Branch**

**388# Gaoxin Road (No.2)**

**East Lake Development Zone**

**Wuhan P. R. China**

**Tel: 400-999-6126**

**E-mail: [market@abclonal.com](mailto:market@abclonal.com)**

**[http: www.abclonal.com.cn](http://www.abclonal.com.cn)**

## Contents

<b>Introduction</b> .....	3
<b>Principle Of The Assay</b> .....	3
<b>Materials Provided</b> .....	4
<b>Sample Collection And Storage</b> .....	6
<b>Precautions For Use</b> .....	6
<b>Experiment Materials</b> .....	7
<b>Reagent Preparation</b> .....	8
<b>Wash Method</b> .....	10
<b>Assay Procedure</b> .....	11
<b>Assay Procedure Summary</b> .....	12
<b>Calculation Of Results</b> .....	13
<b>Typical Data</b> .....	14
<b>Sensitivity</b> .....	15
<b>Specificity</b> .....	15
<b>Precision</b> .....	16
<b>Recovery</b> .....	17
<b>Linearity Dilute</b> .....	18

## Introduction

FKBP1B (FK506 Binding Protein 1B) is a Protein Coding gene. Diseases associated with FKBP1B include Left Ventricular Noncompaction and Catecholaminergic Polymorphic Ventricular Tachycardia. Among its related pathways are Cardiac conduction and Ion channel transport. GO annotations related to this gene include receptor binding and peptidyl-prolyl cis-trans isomerase activity. An important paralog of this gene is MIR6869.

The protein encoded by this gene is a member of the immunophilin protein family, which play a role in immunoregulation and basic cellular processes involving protein folding and trafficking. This encoded protein is a cis-trans prolyl isomerase that binds the immunosuppressants FK506 and rapamycin. It is highly similar to the FK506-binding protein 1A. Its physiological role is thought to be in excitation-contraction coupling in cardiac muscle. There are two alternatively spliced transcript variants of this gene encoding different isoforms.

Has the potential to contribute to the immunosuppressive and toxic effects of FK506 and rapamycin. PPIases accelerate the folding of proteins. It catalyzes the cis-trans isomerization of proline imidic peptide bonds in oligopeptides.

## Principle Of The Assay

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for FKBP1B has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any FKBP1B present is bound by the immobilized antibody. Following incubation unbound samples are removed during a wash step, and then a detection antibody

specific for FKBP1B is added to the wells and binds to the combination of capture antibody-FKBP1B in sample. Following a wash to remove any unbound combination, and enzyme conjugate is added to the wells. Following incubation and wash steps, a substrate is added. A colored product TMB is formed in proportion to the amount of FKBP1B present in the sample. The reaction is terminated by addition of acid and absorbance is measured. A standard curve is prepared from seven FKBP1B standard dilutions and FKBP1B sample concentration determined.

## Materials Provided

Description	Size (192T)	Size (96T)	Size (48T)	Storage	Cat NO.
Human FKBP1B antibody coated plate	(8×12) ×2	8×12	8×6	4°C	RM00368
Human FKBP1B Standard lyophilized	4 vials	2 vials	1 vial	4°C	RM00365
Standard/sample Diluent (R1)	2 bottles ×20 mL	1 bottle ×20 mL	1 bottle ×6 mL	4°C	RM00023

Human FKBP1B concentrated biotin conjugate antibody (100×)	2 vials ×120 µL	1 vial ×120 µL	1 vial ×60 µL	4°C	RM00366
Biotin-Conjugate antibody Diluent (R2)	1 bottle ×32 mL	1 bottle × 16 mL	1 bottle × 10 mL	4°C	RM00024
Streptavidin-HRP concentrated (100×)	2 vials ×120 µL	1 vial ×120 µL	1 vial ×60 µL	4°C	RM00367
Streptavidin-HRP Diluent(R3)	1 bottle ×32 mL	1 bottle ×16 mL	1 bottle ×16 mL	4°C	RM00025
Wash Buffer (20x)	2 bottles ×30 mL	1 bottle × 30 mL	1 bottle ×30 mL	4°C	RM00026
Substrate Solution (Dark)	2 bottles ×12 mL	1 bottle ×12 mL	1 bottle ×6 mL	4°C	RM00027
Stop Solution	1 bottle ×24 mL	1 bottle ×12 mL	1 bottle ×12 mL	4°C	RM00028
Plate Sealers	8 strips	4 strips	2 strips		
Specification	1				

## **Sample Collection And Storage**

**1. Cell Culture Supernates:**

Centrifuge 1000x g for 10 min and detect; or aliquot and store samples at -20°C to -70°C (Stored at 2-8°C if tested within 24 hours). Avoid freeze/thaw cycles.

**2. Serum:**

Use a serum separator tube and allow samples to clot for 30 minutes before centrifugation for 10 minutes at 1000x g, and detect; or aliquot and store samples at -20°C to -70°C (Stored at 2-8°C if tested within 24 hours). Avoid freeze/thaw cycles.

**3. Plasma**

Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge for 15 minutes at 1000x g within 30 minutes of collection, and detect; or aliquot and store samples at -20°C to -70°C (Stored at 2-8°C if tested within 24 hours). Avoid freeze / thaw cycles.

**4. Avoid hemolytic and hyperlipidemia sample for Serum and Plasma.**

**5. Dilution:**

Dilute samples at the appropriate multiple (recommend to do pre-test to determine the dilution factor).

## **Precautions For Use**

- 1. Reagents may be harmful, if ingested, rinse it with an excess amount of tap water.**
- 2. Stop Solution contains strong acid. Wear eye, hand, and face protection.**
- 3. Store the kits at 2 to 8°C before use, throw away the unspent kits.**

4. Apart from the standard of kits, other components should not be refrigerated.
5. Please perform simple centrifugation to collect the liquid before use.
6. Apart from Stop Buffer and Concentrated Wash Buffer can be commonly used, the other components in the kits are specified. Do not mix or substitute reagents with those from other lots or other sources.
7. Adequate mixing is very important for good result. Use a mini-vortexer at the lowest frequency.
8. Mix the sample and all components in the kits adequately, and use clean plastainer to prepare wash buffer.
9. Both the sample and standard should be assayed in duplicate, and the sequence of the reagents should be added consistently.
10. The kit should not be used beyond the expiration date.
11. The kit should be away from light when it is stored or incubated.
12. To reduce the likelihood of blood-borne transmission of infectious agents, handle all serum, plasma and other biological fluids in accordance with NCCLS regulations.
13. To avoid cross contamination, please use disposable pipette tips.
14. Aspirate Stop Solution (100  $\mu$  L/well), mix, determine the optical density of each well within 5 minutes, using a microplate reader set to 450 nm. If wavelength correction is available, set to 570 nm or 630 nm. If wavelength correction is not available, subtract readings at 570 nm or 630 nm from the readings at 450nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate..

## **Experiment Materials**

- 1. ELIASA (measuring absorbance at 450 nm, with the correction wavelength set at 570 nm or 630 nm)**
- 2. Pipettes and pipette tips: 0.5-10, 2-20, 20-200, 200-1000  $\mu$ L**
- 3. Microplate washer, Squirt bottle**
- 4. Micro-oscillator**
- 5. Deionized or double distilled water, graduated cylinder**
- 6. Polypropylene Test tubes for dilution**

## **Reagent Preparation**

- 1. Bring all reagents to room temperature before use. If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved.**
- 2. Wash buffer: 1:20 diluted with double distilled or deionized water before use.**
- 3. Biotin-Conjugate antibody: 1:100 diluted with the Biotin-Conjugate antibody Diluent (R2) before use, and the diluted solution should be used up within 30 min.**

## Dilution Method


Strip	Concentrated Biotin-Conjugate antibody (1:100)	Testing dilution buffer (R2)
2	20	1980
4	40	3960
6	60	5940
8	80	7920
10	100	9900
12	120	11880

4. Streptavidin-HRP: 1:100 diluted with the Streptavidin-HRP Diluent (R3) before use, and the diluted solution should be used up within 30 min.

## Dilution Method

Strip	Concentrated Streptavidin-HRP (1:100)	Testing dilution buffer (R3)
2	20	1980
4	40	3960
6	60	5940
8	80	7920
10	100	9900
12	120	11880

5. **Standard:** Add standard/sample dilution (R1) 1mL into freeze-dried standard, sit for a minimum of 15 minutes with gentle agitation prior to making dilutions (50 ng/mL), then dilute according to the requirement (recommended concentration for standard curve: 50, 25, 12.5, 6.25, 3.125, 1.562, 0.78, 0 ng/mL). Redissolved standard solution (50 ng/mL), aliquot and store at -20°C— -70°C.

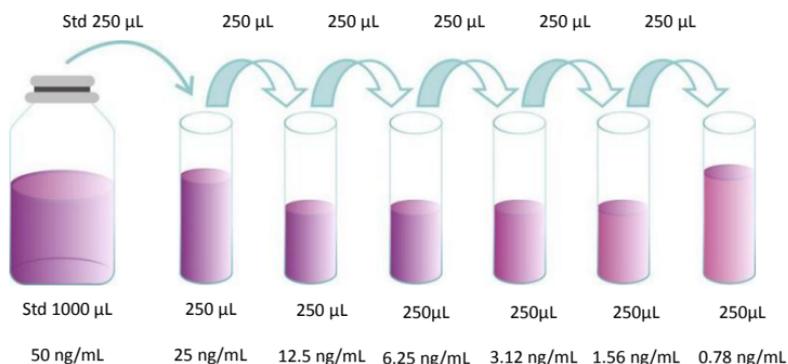

## Wash Method

**Automatic washer:** Add wash buffer 300 µL/well, soak for about 10-20 seconds, and wash 5 times.


**Washer:** Throw all the solutions in the plate well, clean with absorbent paper, and then dispense wash buffer 300 µL/well, throw all the solutions in the plate well after holding 30 seconds, repeat 4 times.

## Assay Procedure

1. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal.
2. Add wash buffer 300  $\mu\text{L}$ /well, aspirate each well after holding 30 seconds, repeating the process three times for a total of four washes. Then use enzyme-marked plate in a short time, do not let it dry.
3. Add 100 $\mu\text{L}$  Standard /Sample Diluent (R1) in blank well.
4. Apart from blank well, add 100  $\mu\text{L}$  different concentration of standard and sample in other wells, cover with the adhesive strip provided. Incubate for 2 hours at room temperature (20 to 25°C)
5. Wash the plate 5 times as in step 2.
6. Prepare the Biotin-Conjugate antibody Working Solution 20 minutes early.
7. Add Biotin-Conjugate antibody diluent (R2) in blank well and Biotin-Conjugate antibody Working Solution in other wells (100  $\mu\text{L}$ /well), cover with new adhesive strip provided, shake with Micro-oscillator (100 r/min). Incubate for 1 hours at room temperature (20 to 25°C)
8. Prepare the Streptavidin-HRP Working Solution 20 minutes early, place away from light at room temperature.
9. Wash the plate 5 times as in step 2.
10. Aspirate Streptavidin-HRP diluent (R3) in blank well and aspirate Streptavidin-HRP Working Solution in other wells (100  $\mu\text{L}$ /well), cover with new adhesive strip provided, shake with Micro-oscillator (100 r/min). Incubate for 30 minutes at room temperature (20 to 25°C)
11. Warm-up the ELIASA.
12. Wash the plate 5 times.

13. Aspirate substrate Solution (100  $\mu\text{L}$ /well). Incubate for 20 minutes at room temperature under dark.
14. Aspirate Stop Solution (100  $\mu\text{L}$ /well), mix, determine the optical density of each well within 5 minutes, using a microplate reader set to 450 nm.

## Assay Procedure Summary

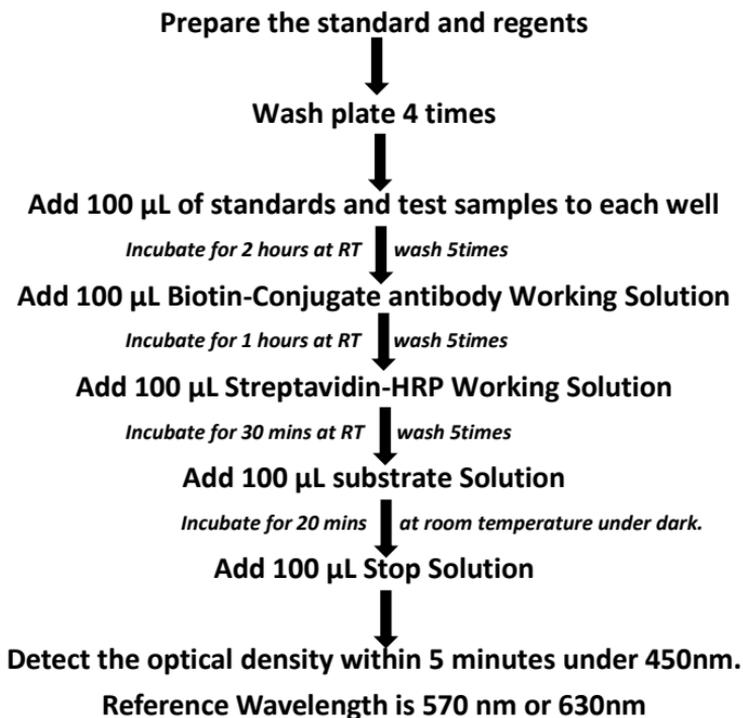


## Calculation Of Results

1. Average the duplicate readings for each standard, control and sample, and subtract the average zero standard optical density (O.D.).
2. Create a standard curve by reducing the data using computer software capable of generating a log/log curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on a log/log graph. The data may be linearized by plotting the log of the FKBP1B concentrations versus the log of the O.D. on a linear scale, and the best fit line can be determined by regression analysis.
3. If the detect result is higher than the standard curve's upper limit, then dilute samples, and the concentration read from the standard curve must be multiplied.

## Typical Data

Standard (ng/mL)	OD value		Average value	Correct value
0	0.045	0.047	0.046	---
0.78	0.078	0.074	0.076	0.03
1.56	0.124	0.128	0.126	0.08
3.12	0.212	0.201	0.2065	0.1605
6.25	0.369	0.321	0.345	0.299
12.5	0.756	0.779	0.7675	0.7215
25	1.523	1.546	1.5345	1.4885
50	2.895	2.859	2.877	2.831

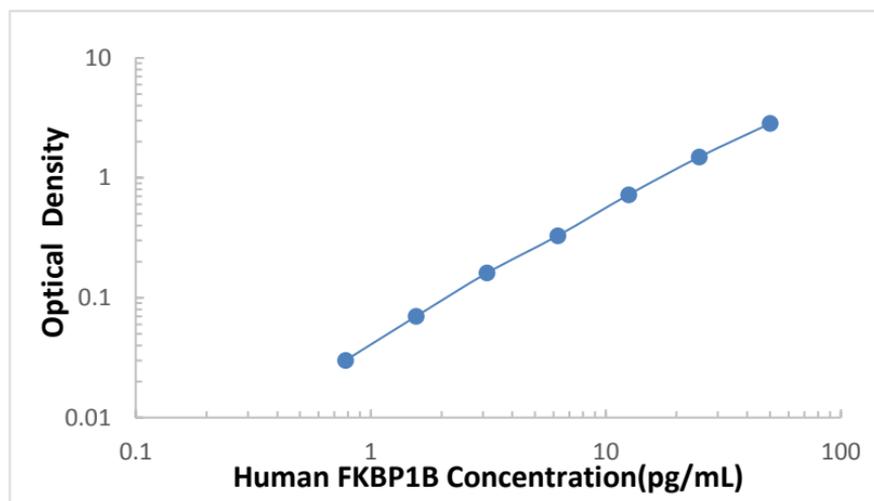

The standard curves are provided for demonstration only. A standard curve should be generated for each set of FKBP1B assayed.

## **Sensitivity**

The minimum detectable dose (MDD) of FKBP1B ranged from 0.2ng/mL. The MDD was determined by adding two standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration.

## **Specificity**

This assay recognizes both recombinant and natural human FKBP1B. Use 100 ng/mL to do specificity assay. No significant cross-reactivity was observed with the following: Other species not determined.

## Precision

### Intra-plate Precision

Repeat 20 times detection of 3 known concentration sample enzyme plate to evaluate the Intra-plate precision.

<b>Sample</b>	<b>1</b>	<b>2</b>	<b>3</b>
<b>Repeat Times</b>	<b>20</b>	<b>20</b>	<b>20</b>
<b>Average Value (ng/mL)</b>	<b>2.0</b>	<b>10</b>	<b>20</b>
<b>Standard Deviation (SD)</b>	<b>0.046</b>	<b>0.35</b>	<b>0.74</b>
<b>Variable Coefficient CV (%)</b>	<b>2.3</b>	<b>3.5</b>	<b>3.7</b>

## Inter-plate Precision

Repeat 20 times detection of 3 known concentration sample enzyme plate to evaluate the Inter-plate precision.

Sample	1	2	3
Repeat Times	20	20	20
Average Value (ng/mL)	2.0	10	20
Standard Deviation (SD)	0.136	0.73	1.28
Variable Coefficient CV (%)	6.8	7.3	6.4

## Recovery

Aspirate 3 different concentration of human FKBP1B into healthy human serum and plasma, calculate the recovery.

Sample Form	Average Recover (%)	Range (%)
Serum	102	87-113
Plasma	103	90-118

## Linearity Dilute

Aspirate high concentration of human FKBP1B into 4 healthy human serum, dilute in the range of standard curve kinetics and evaluate the linearity.

<b>Dilution</b>	<b>Average Value (%)</b>	<b>Range (%)</b>
<b>1:2</b>	<b>102</b>	<b>85-106</b>
<b>1:4</b>	<b>101</b>	<b>90-102</b>
<b>1:8</b>	<b>102</b>	<b>91-112</b>
<b>1:16</b>	<b>103</b>	<b>90-108</b>

